



Client Redline Bio Labs

Analyzed 08/24/2026

This Certificate of Analysis certifies that the sample listed herein was tested by SteriGenix using validated analytical methods and was found to meet the stated specifications at the time of analysis.

SAMPLE INFORMATION

Product	B12	Form	LIQUID
Batch	SGX-RBL-2026-0814-H29	Labeled Qty	10ML
Mol. Formula	C63H88CoN14O14P	CAS Number	68-19-9
Cap Color	Clear	Crimp Color	Copper
Appearance	Red Liquid		

TEST RESULTS

	REFERENCE STANDARD	RESULT	
Identity Confirmation (LC-MS)	B12 (Cyanocobalamin)	B12 (Cyanocobalamin)	✓
Batch Avg Purity (HPLC)	(>98%)	99.38	✓
Net Peptide Content	10ML ± 10%	PASS	✓

HEAVY METAL SCREENING


Not Tested.

BATCH CONFORMITY RESULTS

Not Tested.

HPLC CHROMATOGRAM

HPLC CHROMATOGRAM · B12	DETECTOR: UV 214 NM · 08/24/2026

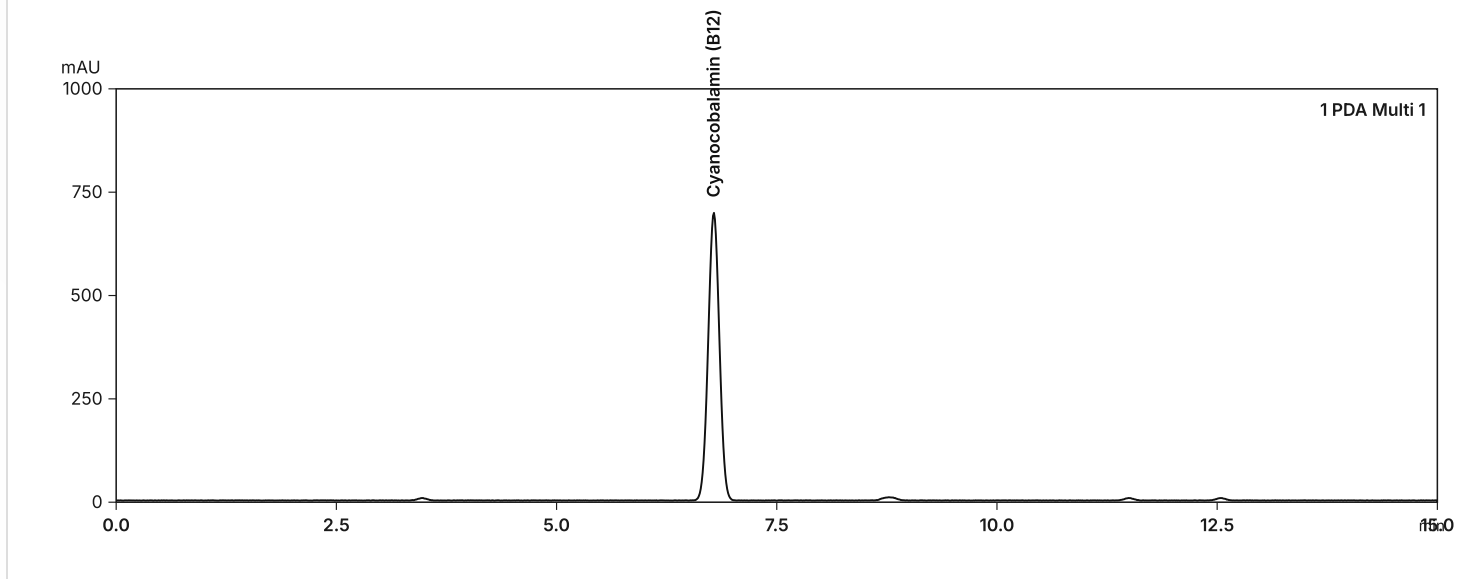

SAMPLE PHOTOS



Dr. R. Caldwell

ANALYST
ID: AN-3271

Dr. P. Anderson

QC REVIEWER
ID: QR-5418

Dr. H. Whitman

QA DIRECTOR
ID: QA-1090



sterigenixanalytical.com/verify

Report#: RPT-2026-534284
Access Code: SGX-RBL-2026-0814-H29

